


Bayer Radiology Data Flow Overview

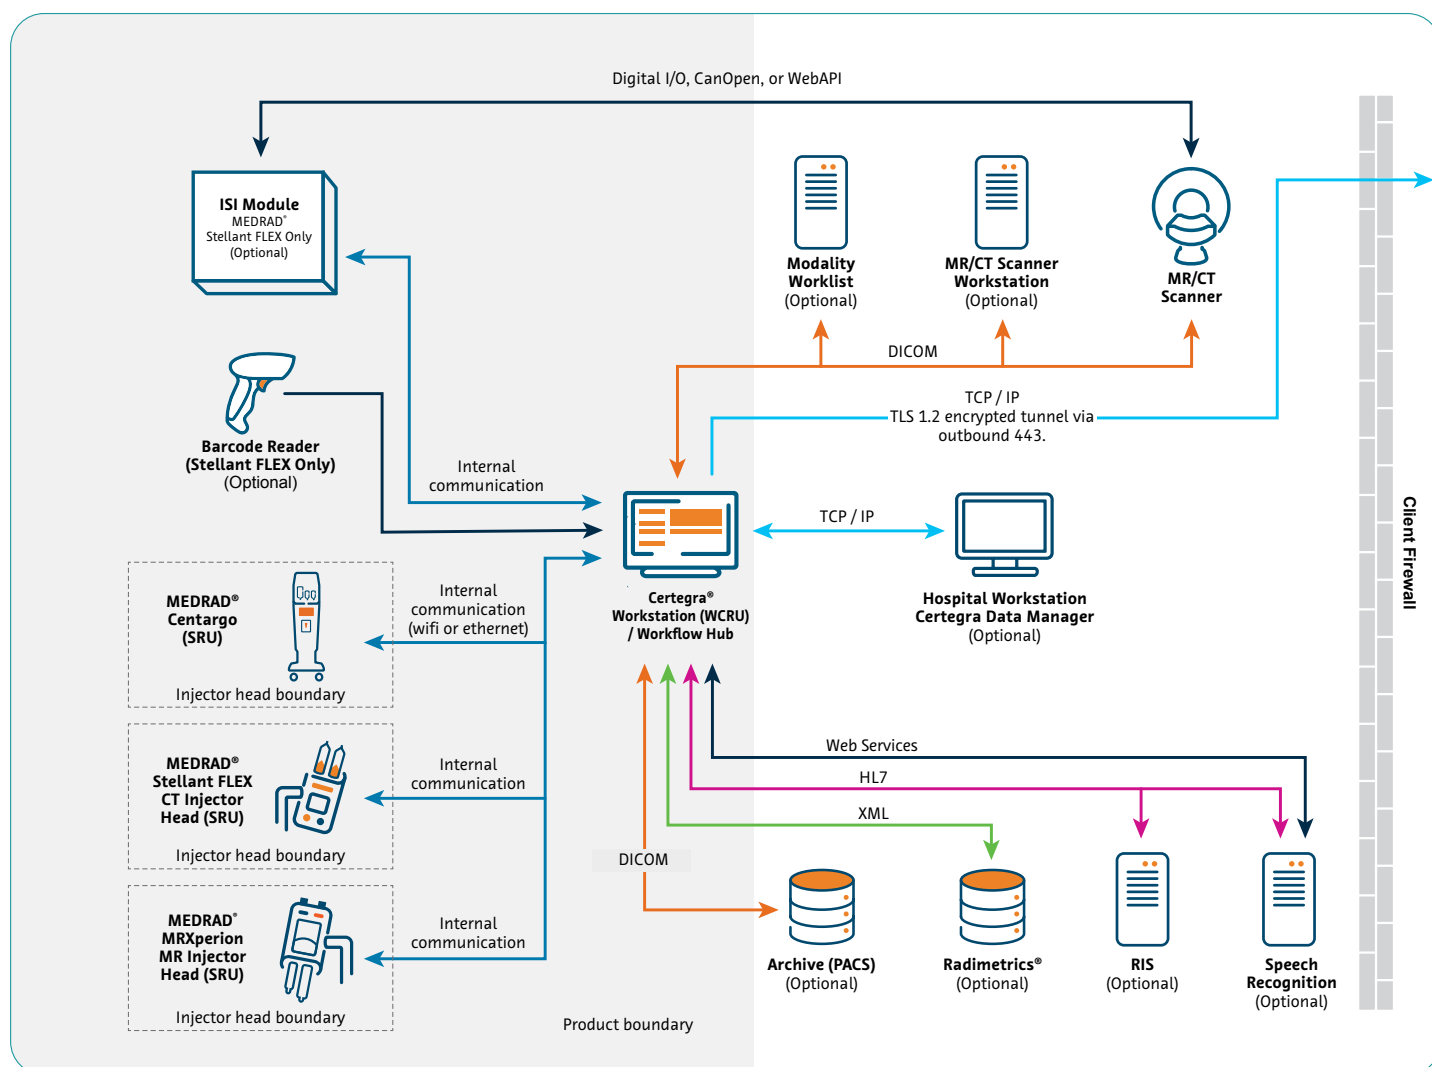

LEGEND

- TCP / IP
- HL7
- DICOM
- XML
- Digital I/O, CanOpen, or Web API
- Internal communication
- CT and MR Suite

Bayer reserves the right to modify the specifications and features described herein or to discontinue any product or service identified in this publication at any time without prior notice or obligation. Please contact your authorized Bayer representative for the most current information.

Bayer, the Bayer Cross, MEDRAD, MEDRAD Stellant FLEX, MEDRAD MRXperion, MEDRAD Centargo, Stellant FLEX, MRXperion, Centargo, Radimetrics, Certegra and Cortenic are trademarks owned by and/or registered to Bayer in the U.S. and/or other countries. Other trademarks and company names mentioned herein are properties of their respective owners and are used herein solely for informational purposes. No relationship or endorsement should be inferred or implied.

© 2025 Bayer. This material may not be reproduced, displayed, modified or distributed without the express prior written consent of Bayer.



Bayer HealthCare LLC
100 Bayer Boulevard
P.O. Box 915
Whippany, NJ 07981
U.S.A.
Phone: +1-412-767-2400
+1-800-633-7231
Fax: +1-412-767-4120
More information on
radiologysolutions.bayer.com



Manufacturer
Bayer Medical Care Inc.
1 Bayer Drive
Indianola, PA 15051-0780
U.S.A.
Phone: +1-412-767-2400
+1-800-633-7231
Fax: +1-412-767-4120

Our dedicated Bayer Cybersecurity Team
and subject matter experts in healthcare
IT are available to answer your questions
and support site specific needs.

[Click here to contact our dedicated
Bayer Cybersecurity Team >](#)